

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0042
Location: HIGHTSTOWN POLICE
Calibration File No.: 00781 Calib. Date: 03/01/2012 Calib. No.: 00018
Certification File No.: 00782 Cert. Date: 03/01/2012 Cert. No.: 00014
Linearity File No.: 00783 Lin. Date: 03/01/2012 Lin. No.: 00014
Solution File No.: 00798 Soln. Date: 04/20/2012 Soln. No.: 00128
Sequential File No.: 00798 File Date: 04/20/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0182
Control Solution %: 0.100% Expires: 07/07/2013
Solution Control Lot: 11G093 Bottle No.: 0889

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:53D		
Control 1 EC	0.100%	18:54D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	18:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:55D		
Control 2 EC	0.099%	18:55D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	18:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:56D		
Control 3 EC	0.099%	18:57D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:58D		

All tests within acceptable tolerance.

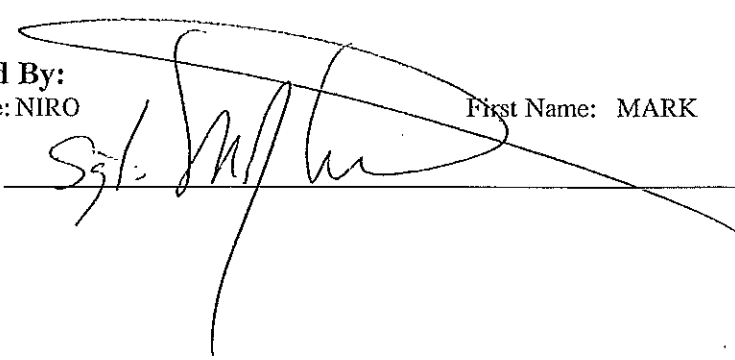
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: NIRO

First Name: MARK

MI: J

Signature: 

Badge No.: 1114

Date: 04/20/2012