

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0042
Location:	HIGHTSTOWN POLICE	
Calibration File No.:	01070	Calib. Date: 09/02/2014
Certification File No.:	01071	Calib. No.: 00025
Linearity File No.:	01072	Cert. Date: 09/02/2014
Solution File No.:	01082	Cert. No.: 00020
Sequential File No.:	01082	Lin. Date: 09/02/2014
		Lin. No.: 00020
		Soln. Date: 11/04/2014
		Soln. No.: 00176
		File Date: 11/04/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0183
Solution Control Lot:	14F130	Expires: 06/20/2016
		Bottle No.: 0065

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:14S		
Control 1 EC	0.102%	15:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	15:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:16S		
Control 2 EC	0.101%	15:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	15:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:17S		
Control 3 EC	0.101%	15:18S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	15:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MILLER

First Name: BENJAMIN

MI: L

Signature: _____

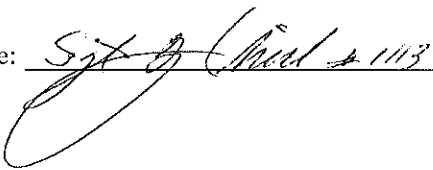

Badge No.: 1113

Date: 11/04/2014