

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0042  
Location: HIGHTSTOWN POLICE  
Calibration File No.: 00942 Calib. Date: 09/13/2013 Calib. No.: 00022  
Certification File No.: 00943 Cert. Date: 09/13/2013 Cert. No.: 00017  
Linearity File No.: 00944 Lin. Date: 09/13/2013 Lin. No.: 00017  
Solution File No.: 00972 Soln. Date: 01/01/2014 Soln. No.: 00162  
Sequential File No.: 00972 File Date: 01/01/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0182  
Control Solution %: 0.100% Expires: 09/13/2014  
Solution Control Lot: 121107 Bottle No.: 0865

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:25S		
Control 1 EC	0.099%	23:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	23:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:27S		
Control 2 EC	0.098%	23:28S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:28S		
Control 3 EC	0.099%	23:29S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:30S		

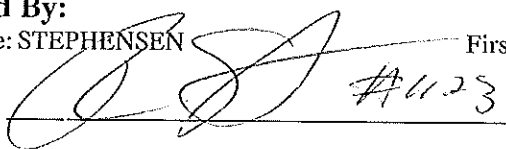
All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: STEPHENSEN First Name: PTL

MI: R

Signature:  #1123

Badge No.: 1123

Date: 01/01/2014