

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0042
Location:	HIGHTSTOWN POLICE	
Calibration File No.:	00942	Calib. Date: 09/13/2013
Certification File No.:	00943	Calib. No.: 00022
Linearity File No.:	00944	Cert. Date: 09/13/2013
Solution File No.:	00986	Cert. No.: 00017
Sequential File No.:	00986	Lin. Date: 09/13/2013
		Lin. No.: 00017
		Soln. Date: 02/25/2014
		Soln. No.: 00164
		File Date: 02/25/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0182
Solution Control Lot:	L2II07	Expires: 09/13/2014
		Bottle No.: 0864

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:50S		
Control 1 EC	0.099%	06:51S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:51S		
Control 2 EC	0.097%	06:52S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	06:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:53S		
Control 3 EC	0.098%	06:54S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	06:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: NIRO

First Name: SGT

MI: J

Signature: \_\_\_\_\_

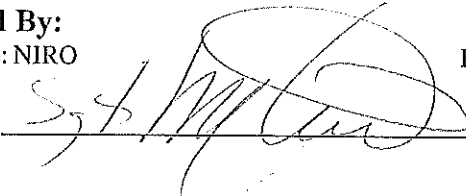

1114

Badge No.: 1114

Date: 02/25/2014