

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0042
Location:	HIGHTSTOWN POLICE		
Calibration File No.:	00942	Calib. Date:	09/13/2013
Certification File No.:	00943	Calib. No.:	00022
Linearity File No.:	00944	Cert. Date:	09/13/2013
Solution File No.:	00977	Cert. No.:	00017
Sequential File No.:	00977	Lin. Date:	09/13/2013
		Lin. No.:	00017
		Soln. Date:	01/22/2014
		Soln. No.:	00163
		File Date:	01/22/2014

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUL S3-0182
Control Solution %:	0.100%			Expires:	09/13/2014
Solution Control Lot:	121107			Bottle No.:	0858

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:50S		
Control 1 EC	0.098%	14:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:51S		
Control 2 EC	0.098%	14:52S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:52S		
Control 3 EC	0.098%	14:53S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:54S		

All tests within acceptable tolerance.

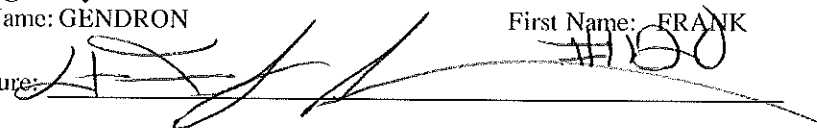
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GENDRON

First Name: FRANK

MI: G

Signature: 

Badge No.: 1120

Date: 01/22/2014