

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0042
Location:	HIGHTSTOWN POLICE	
Calibration File No.:	00994	Calib. Date: 03/13/2014
Certification File No.:	00995	Cert. No.: 00024
Linearity File No.:	00996	Cert. Date: 03/13/2014
Solution File No.:	01007	Lin. Date: 03/13/2014
Sequential File No.:	01007	Lin. No.: 00019
		Soln. Date: 03/30/2014
		Soln. No.: 00166
		File Date: 03/30/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0182
Solution Control Lot:	12I107	Expires: 09/13/2014
		Bottle No.: 0859

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:49S		
Control 1 EC	0.097%	17:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	17:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:51S		
Control 2 EC	0.097%	17:52S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	17:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:52S		
Control 3 EC	0.097%	17:53S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	17:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: NIRO

First Name: MARK

MI: J

Signature: _____

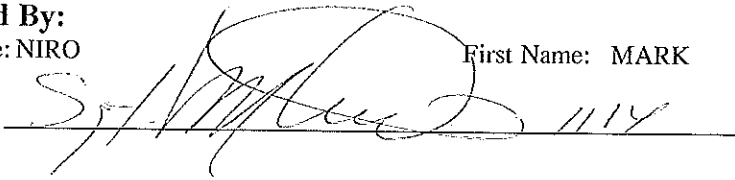

Badge No.: 1114

Date: 03/30/2014