

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0042
Location:	HIGHTSTOWN POLICE	Calib. No.:	00024
Calibration File No.:	00994	Calib. Date:	03/13/2014
Certification File No.:	00995	Cert. Date:	03/13/2014
Linearity File No.:	00996	Lin. Date:	03/13/2014
Solution File No.:	01047	Soln. Date:	06/20/2014
Sequential File No.:	01047	File Date:	06/20/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0183
Solution Control Lot:	12K108	Expires:	11/05/2014
		Bottle No.:	0117

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:31D		
Control 1 EC	0.098%	14:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	14:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:32D		
Control 2 EC	0.097%	14:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	14:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:33D		
Control 3 EC	0.097%	14:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	14:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: NIRO

First Name: SGT

MI: J

Signature: _____

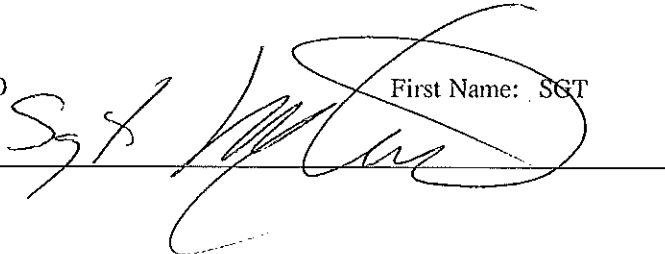

Badge No.: 1114

Date: 06/20/2014