

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0042
Location: HIGHTSTOWN POLICE
Calibration File No.: 00994 Calib. Date: 03/13/2014 Calib. No.: 00024
Certification File No.: 00995 Cert. Date: 03/13/2014 Cert. No.: 00019
Linearity File No.: 00996 Lin. Date: 03/13/2014 Lin. No.: 00019
Solution File No.: 01055 Soln. Date: 07/19/2014 Soln. No.: 00172
Sequential File No.: 01055 File Date: 07/19/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0183
Control Solution %: 0.100% Expires: 11/05/2014
Solution Control Lot: 12K108 Bottle No.: 1172

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 16:38D | | |
| Control 1 EC | 0.099% | 16:39D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.097% | 16:39D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:39D | | |
| Control 2 EC | 0.097% | 16:40D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.097% | 16:40D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:41D | | |
| Control 3 EC | 0.097% | 16:41D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.098% | 16:41D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:42D | | |

All tests within acceptable tolerance.

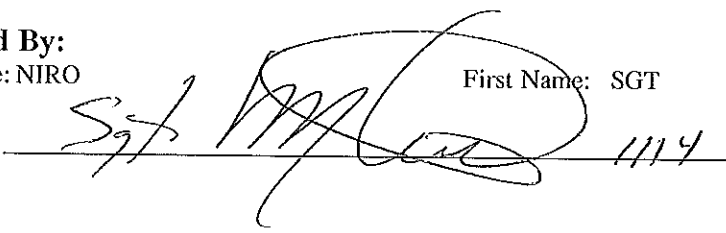
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: NIRO

First Name: SGT

MI: J

Signature:  1114

Badge No.: 1114

Date: 07/19/2014