

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARTN-0042 |
| Location: | HIGHTSTOWN POLICE | |
| Calibration File No.: | 01284 | Calib. Date: 08/07/2017 |
| Certification File No.: | 01285 | Calib. No.: 00032 |
| Linearity File No.: | 01286 | Cert. Date: 08/07/2017 |
| Solution File No.: | 01297 | Cert. No.: 00027 |
| Sequential File No.: | 01297 | Lin. Date: 08/07/2017 |
| | | Lin. No.: 00027 |
| | | Soln. Date: 09/25/2017 |
| | | Soln. No.: 00224 |
| | | File Date: 09/25/2017 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDUL S3-0183 |
| Solution Control Lot: | 17050 | Expires: 01/30/2019 |
| | | Bottle No.: 0936 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 13:49D | | |
| Control 1 EC | 0.099% | 13:50D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 13:50D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:51D | | |
| Control 2 EC | 0.098% | 13:52D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 13:52D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:52D | | |
| Control 3 EC | 0.099% | 13:53D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 13:53D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:54D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MILLER

First Name: BENJAMIN

MI: L

Signature: _____

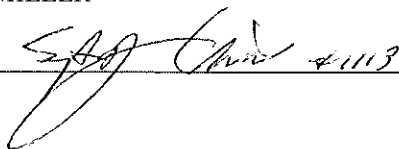

Badge No.: 1113

Date: 09/25/2017