

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0042  
Location: HIGHTSTOWN POLICE  
Calibration File No.: 01405 Calib. Date: 11/28/2018 Calib. No.: 00035  
Certification File No.: 01406 Cert. Date: 11/28/2018 Cert. No.: 00030  
Linearity File No.: 01407 Lin. Date: 11/28/2018 Lin. No.: 00030  
Solution File No.: 01418 Soln. Date: 01/19/2019 Soln. No.: 00248  
Sequential File No.: 01418 File Date: 01/19/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0183  
Control Solution %: 0.100% Expires: 01/31/2020  
Solution Control Lot: 18050 Bottle No.: 0866

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:40S		
Control 1 EC	0.101%	12:40S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:41S		
Control 2 EC	0.100%	12:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:43S		
Control 3 EC	0.100%	12:44S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:44S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:45S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


### Changed By:

Last Name: STEPHENSEN

First Name: SGT

MI: R

Signature: \_\_\_\_\_

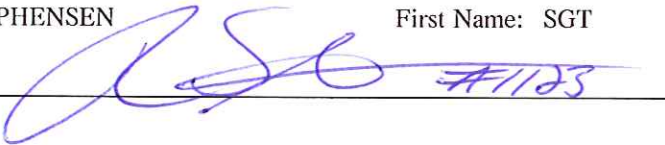

Badge No.: 1123

Date: 01/19/2019