

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0042
Location:	HIGHTSTOWN POLICE	Calib. No.:	00037
Calibration File No.:	01477	Cert. Date:	10/04/2019
Certification File No.:	01478	Lin. Date:	10/04/2019
Linearity File No.:	01479	Soln. Date:	11/28/2019
Solution File No.:	01492	File Date:	11/28/2019
Sequential File No.:	01492		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0183
Solution Control Lot:	19020	Expires:	01/08/2021
		Bottle No.:	0559

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:00S		
Control 1 EC	-.---%	20:01S	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	20:01S	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: STEPHENSEN

First Name: SGT

MI: R

Signature: _____

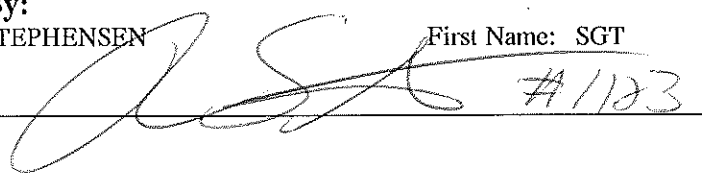

Badge No.: 1123

Date: 11/28/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0042
Location:	HIGHTSTOWN POLICE	Calib. No.:	00037
Calibration File No.:	01477	Cert. Date:	10/04/2019
Certification File No.:	01478	Lin. Date:	10/04/2019
Linearity File No.:	01479	Soln. Date:	11/28/2019
Solution File No.:	01493	File Date:	11/28/2019
Sequential File No.:	01493		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUL S3-0183
Control Solution %:	0.100%			Expires:	01/08/2021
Solution Control Lot:	19020			Bottle No.:	0524

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:10S		
Control 1 EC	0.100%	22:11S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:11S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:11S		
Control 2 EC	0.098%	22:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	22:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:13S		
Control 3 EC	0.099%	22:14S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	22:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:14S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: STEPHENSEN

First Name: SGT

MI: R

Signature: _____



Badge No.: 1123

Date: 11/28/2019