

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0042  
Location: HIGHTSTOWN POLICE  
Calibration File No.: 01687 Calib. Date: 01/13/2023 Calib. No.: 00046  
Certification File No.: 01688 Cert. Date: 01/13/2023 Cert. No.: 00041  
Linearity File No.: 01689 Lin. Date: 01/13/2023 Lin. No.: 00041  
Solution File No.: 01696 Soln. Date: 03/14/2023 Soln. No.: 00315  
Sequential File No.: 01696 File Date: 03/14/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0183  
Control Solution %: 0.100% Expires: 04/04/2024  
Solution Control Lot: 22110 Bottle No.: 0890

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:44S		
Control 1 EC	0.102%	05:45S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	05:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:46S		
Control 2 EC	0.098%	05:47S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	05:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:48S		
Control 3 EC	0.099%	05:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	05:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:50S		

All tests within acceptable tolerance.

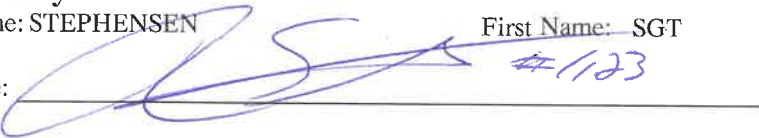
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: STEPHENSEN

First Name: SGT

MI: R

Signature: 

Badge No.: 1123

Date: 03/14/2023